

Table1

Nominal size	2R
Overflow capacity ml	4 ± 0.5
a	1
d1	16 ± 0.15
d2	13 ^{+0.2} _{-0.3}
d3	max. 10.5
d4	7 ± 0.2
h1	35 ± 0.5
h2	min. 22
h3	8 ± 0.5
r1	2.5
r2	1.5
S1	1 ± 0.04
S2	min. 0.6
t	max. 0.7

Vial ISO 8362-1:2009

Size designation of injection vial :2R

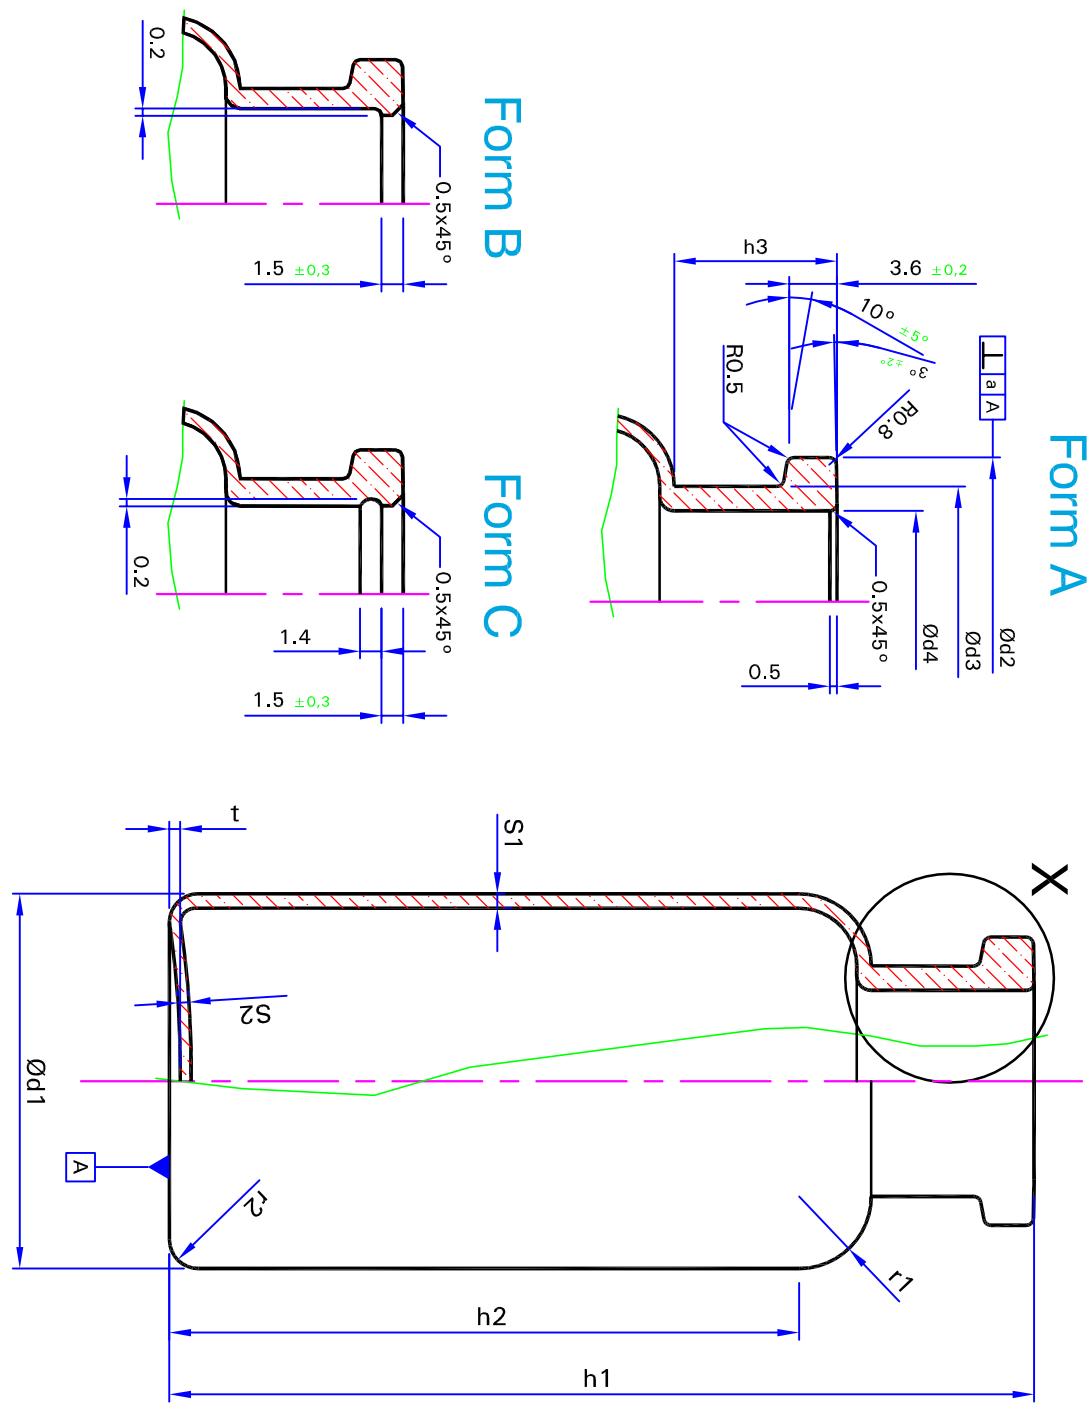


Table 1

Nominal size	4R
Overflow capacity ml	6 ± 0.5
a	1
d1	16 ± 0.15
d2	13 ^{+0.2} _{-0.3}
d3	max. 10.5
d4	7 ± 0.2
h1	45 ± 0.5
h2	min. 32
h3	8 ± 0.5
r1	2.5
r2	1.5
S1	1 ± 0.04
S2	min. 0.6
t	max. 0.7

Vial ISO 8362-1:2009

Size designation of injection vial :4R

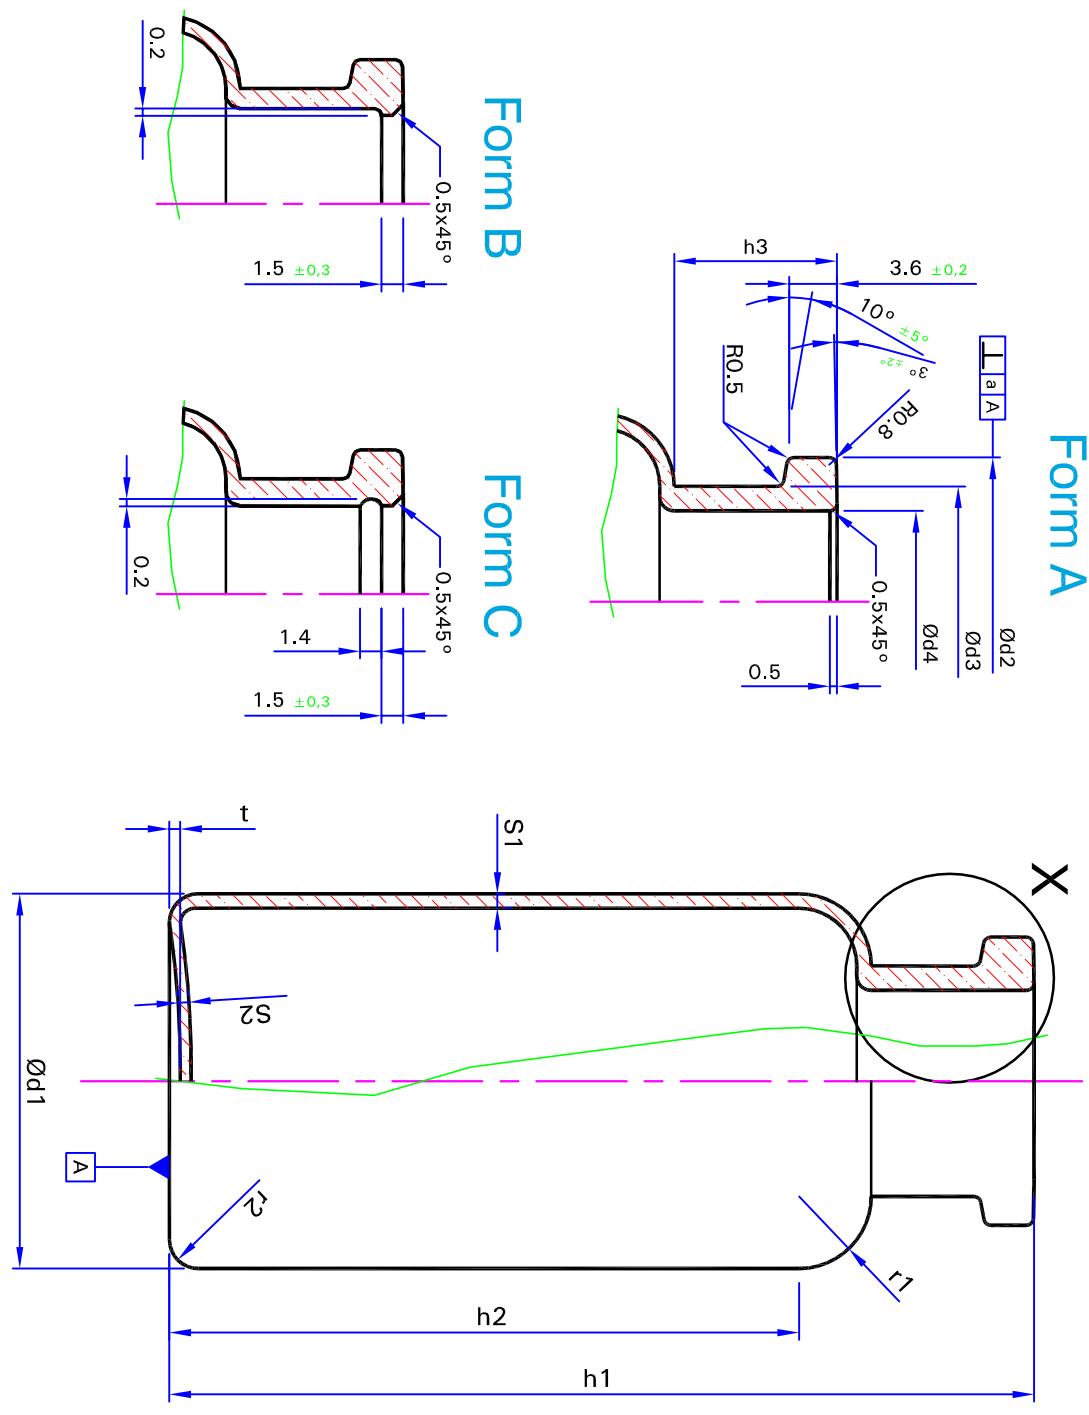


Table 1

Nominal size	6R
Overflow capacity m	10 ± 0.5
a	1.2
d1	22 ± 0.2
d2	20 +0.2 -0.3
d3	16.5
d4	12.6 ± 0.2
h1	40 ± 0.5
h2	min. 26
h3	8.5 ± 0.5
r1	3.5
r2	2
S1	1 ± 0.04
S2	min. 0.7
t	max. 0.7

Vial ISO 8362-1:2009



MOODY
 INTERNATIONAL



NACI

National Accreditation Center of Iran
 مرکز ملی تایید صلاحیت ایران


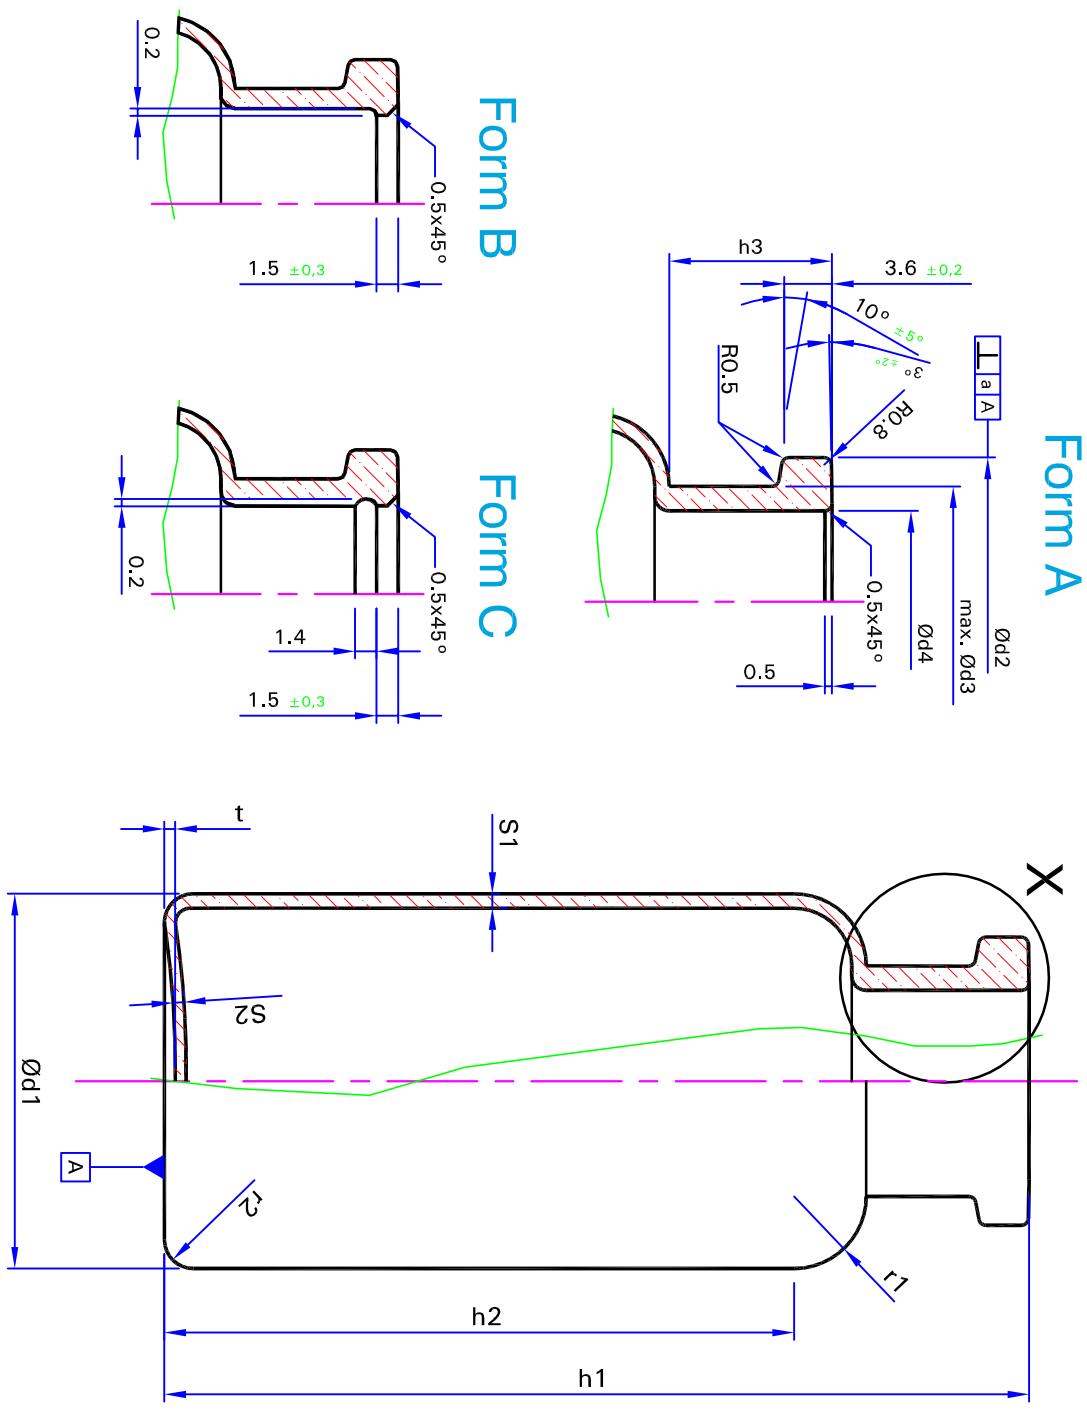


Table1

Nominal size	8R
Overflow capacity ml	11.5 ± 0.5
a	1.2
d1	22 ± 0.2
d2	$20^{+0.2}_{-0.3}$
d3	max. 16.5
d4	12.6 ± 0.2
h1	45 ± 0.5
h2	min. 31
h3	8.5 ± 0.5
r1	3.5
r2	2
S1	1 ± 0.04
S2	min. 0.7
t	max. 0.7

Vial ISO 8362-1:2009

Size designation of injection vial :8R

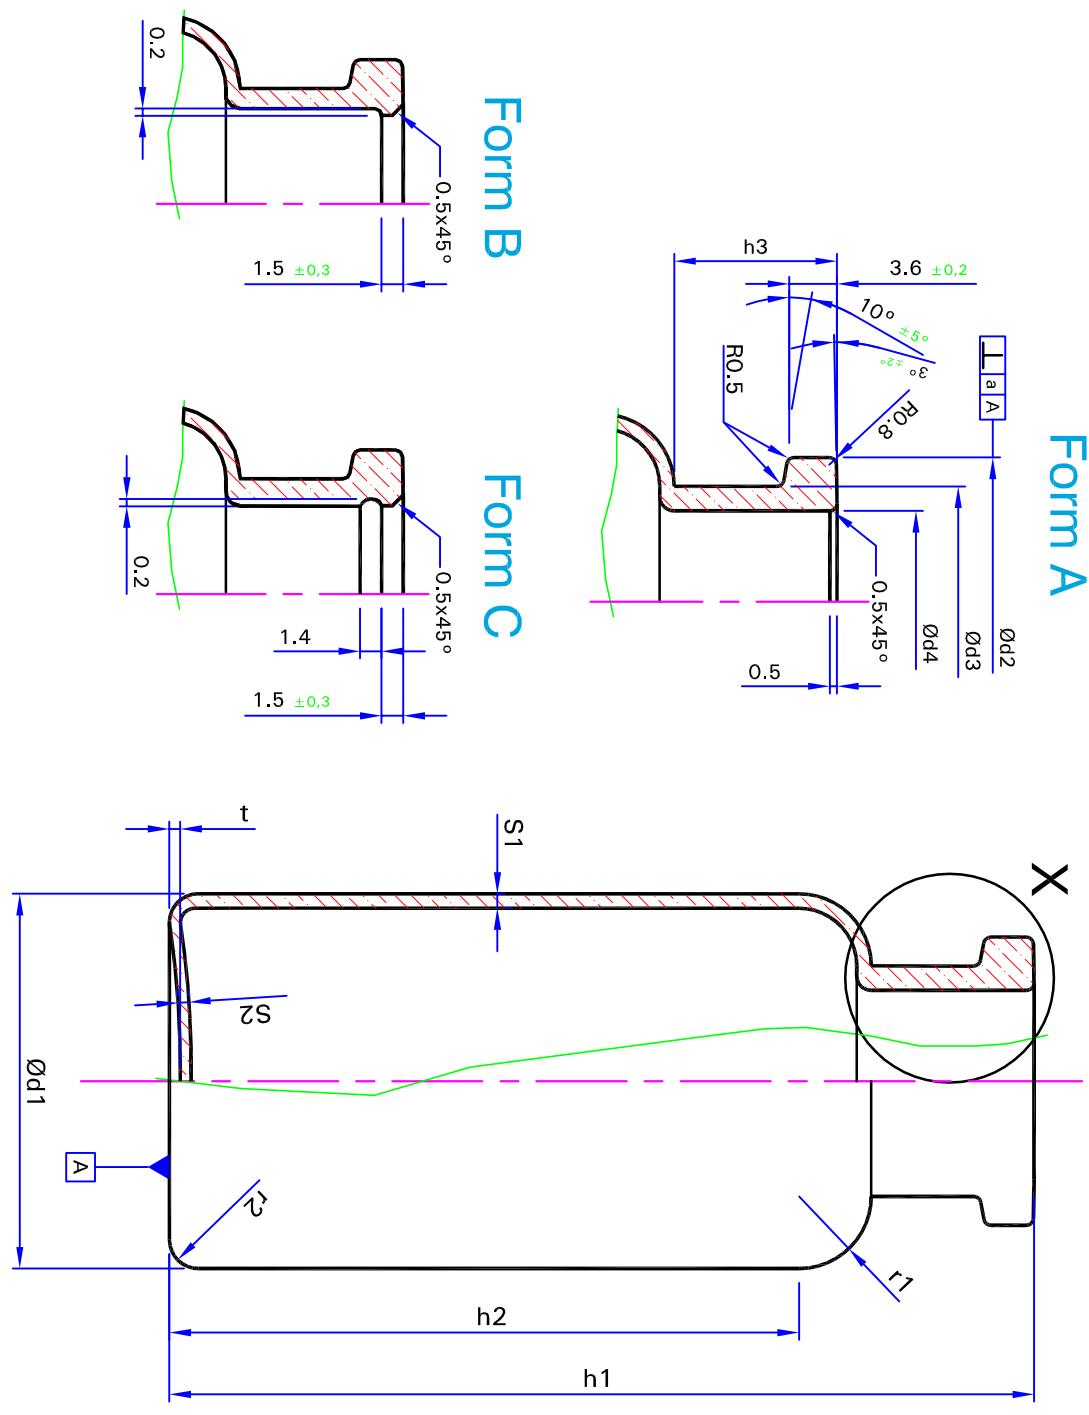


Injection vial

Table1

Nominal size	10R
Overflow capacity ml	13.5 ± 1
a	1.2
d1	24 ± 0.2
d2	20 $^{+0.2}_{-0.3}$
d3	max. 16.5
d4	12.6 ± 0.2
h1	45 ± 0.5
h2	min. 30
h3	9 ± 0.5
r1	4.0
r2	2
S1	1 ± 0.04
S2	min. 0.7
t	max. 0.7

Vial ISO 8362-1:2009

Size designation of injection vial :10R

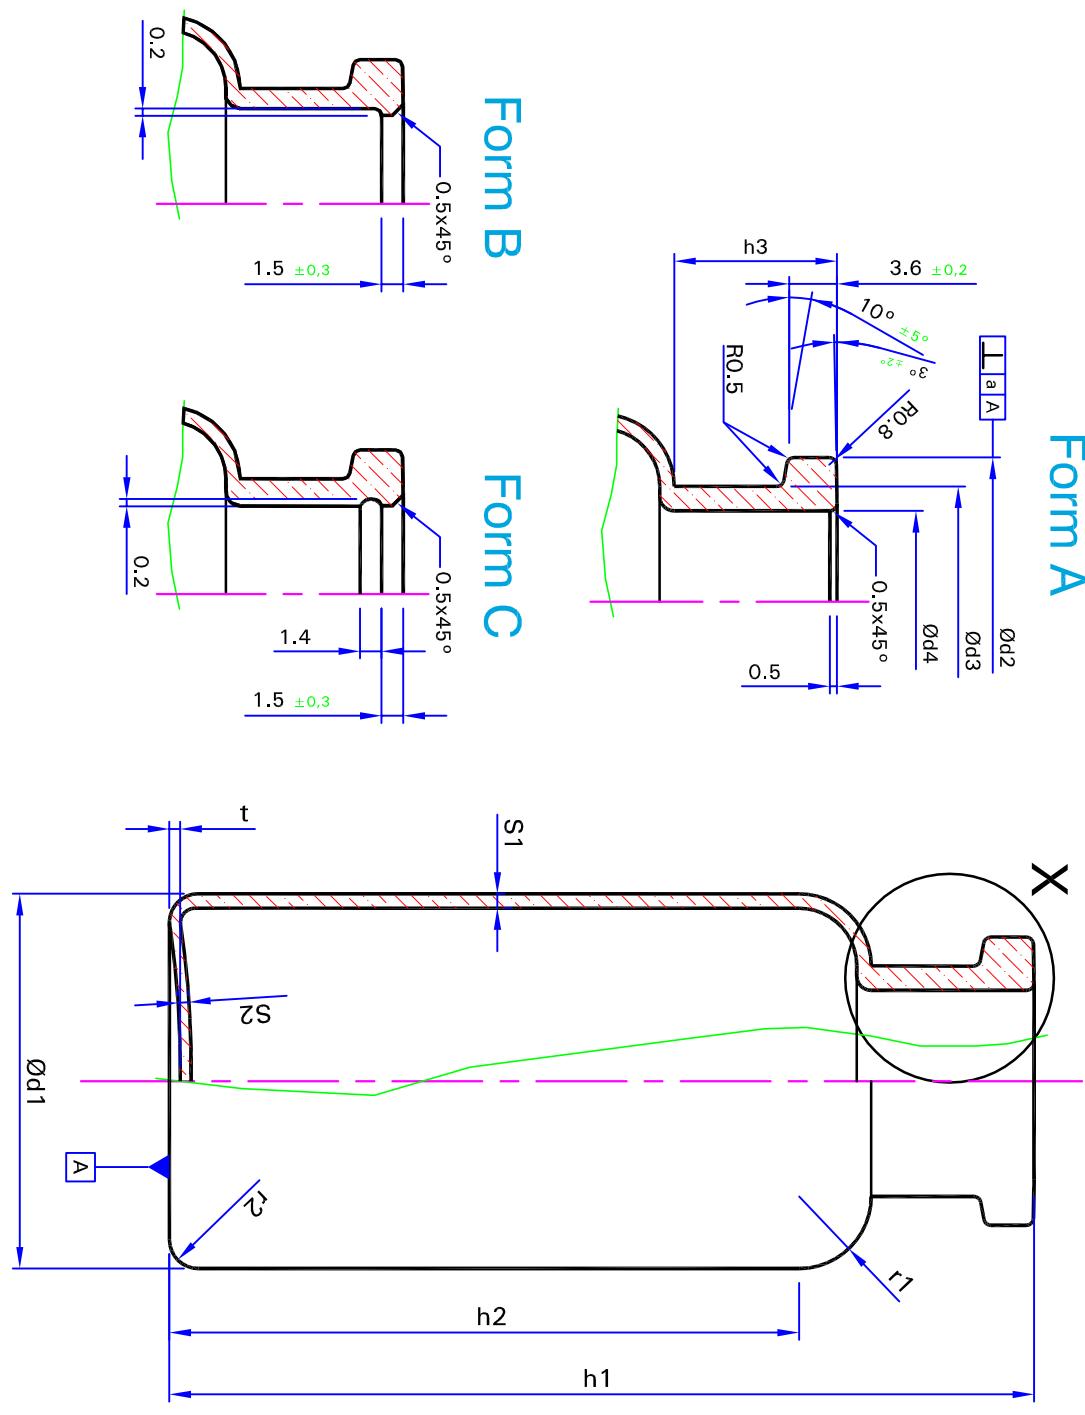

Injection vial

Table1

Nominal size	15R
Overflow capacity ml	19 ± 1
a	1.2
d1	24 ± 0.2
d2	20 +0.2 - 0.3
d3	max. 16.5
d4	12.6 ± 0.2
h1	60 ± 0.5
h2	min. 45
h3	9 ± 0.5
r1	4.0
r2	2
S1	1 ± 0.04
S2	min. 0.7
t	max. 0.7

Vial ISO 8362-1:2009

Size designation of injection vial :15R


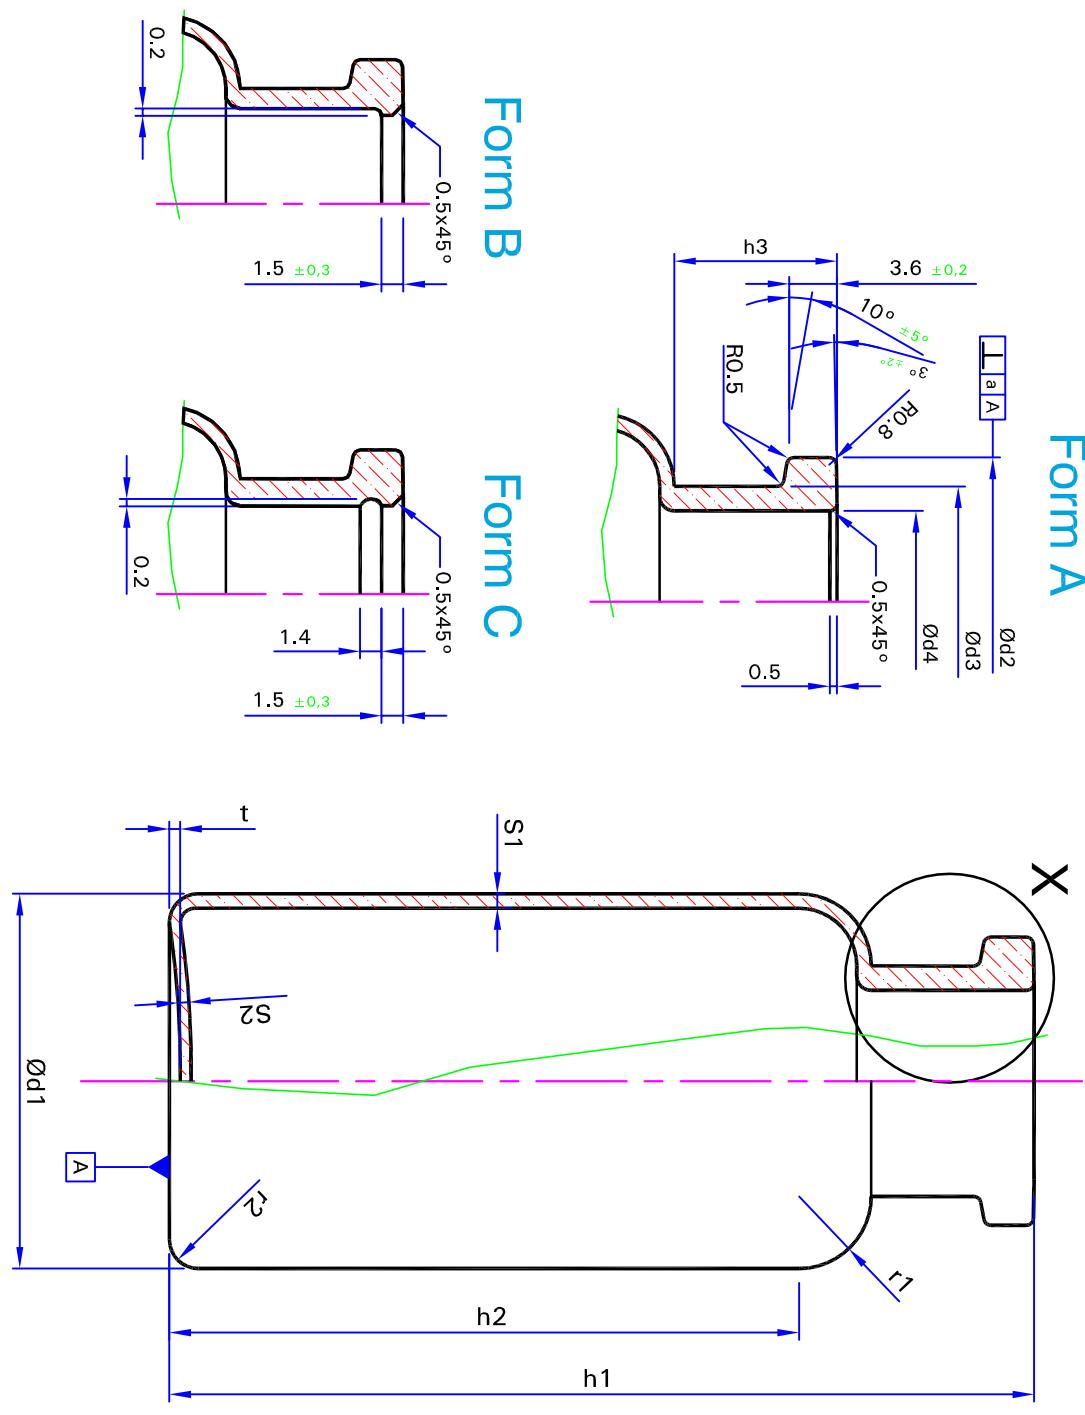


Table1

Nominal size	20R
Overflow capacity ml	26 ± 1.5
a	1.5
d1	30 ± 0.25
d2	20 +0.2 -0.3
d3	max. 17.5
d4	12.6 ± 0.2
h1	55 ± 0.7
h2	min. 35
h3	10 ± 0.75
r1	5.5
r2	2.5
S1	1.2 ± 0.05
S2	min. 0.7
t	max. 1

Vial ISO 8362-1:2009

Size designation of injection vial :20R

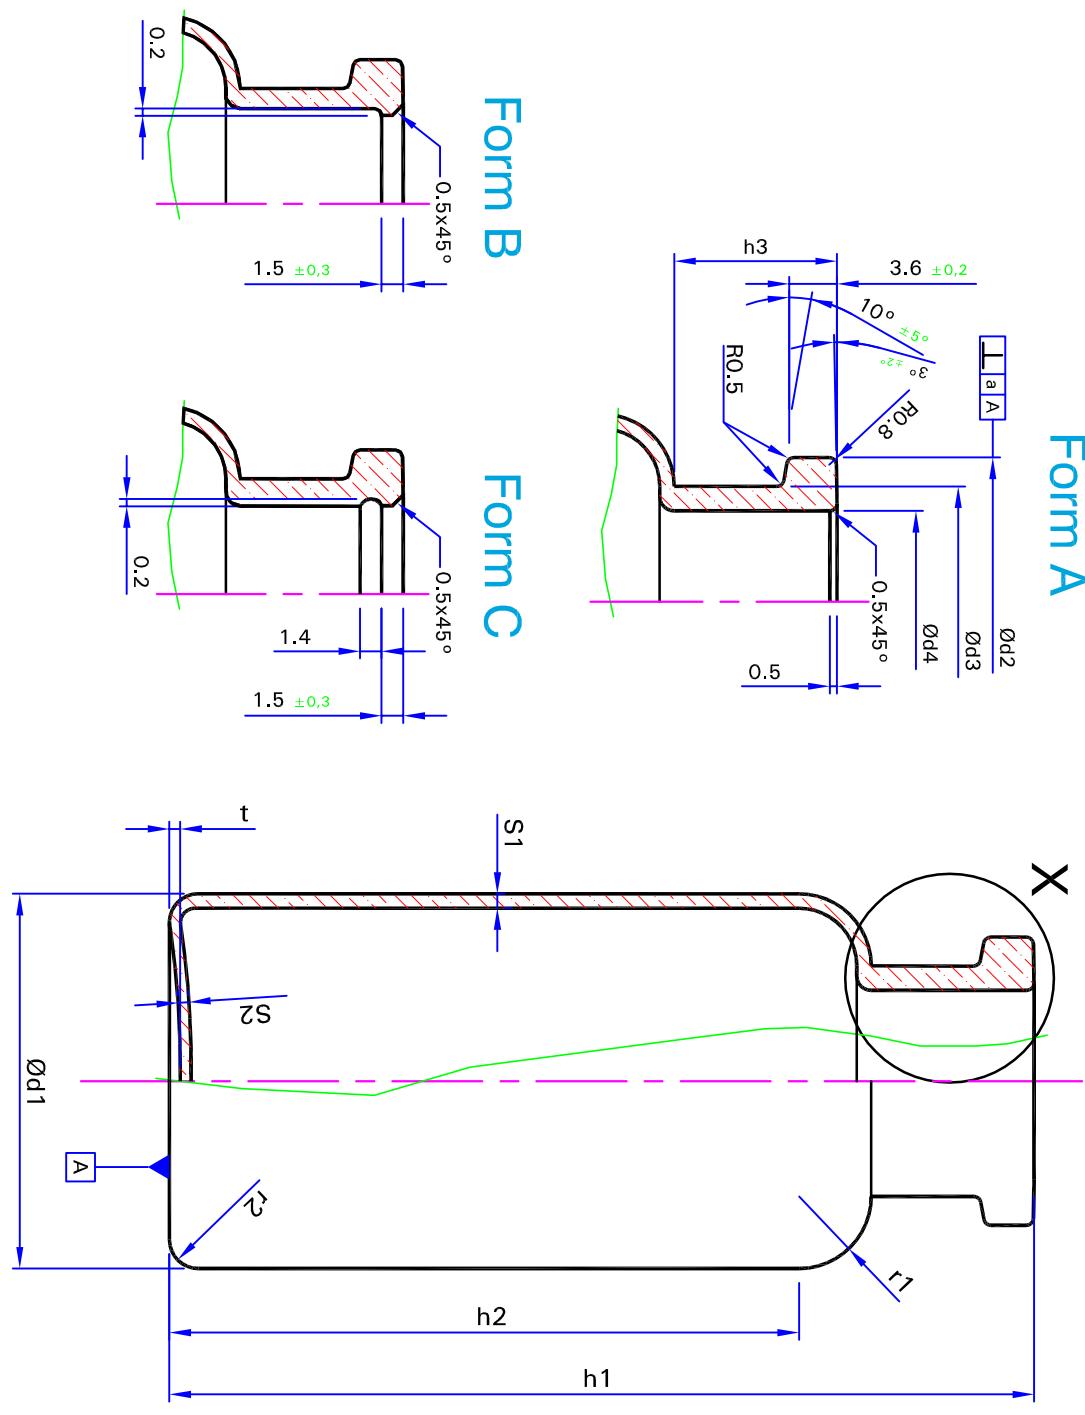

Injection vial

Table1

Nominal size	25R
Overflow capacity ml	32.5 ± 1.5
a	1.5
d1	30 ± 0.25
d2	20 ^{+0.2} _{-0.3}
d3	max. 17.5
d4	12.6 ± 0.2
h1	65 ± 0.7
h2	min. 45
h3	10 ± 0.75
r1	5.5
r2	2.5
S1	1.2 ± 0.05
S2	min. 0.7
t	max. 1

Vial ISO 8362-1:2009

Size designation of injection vial :25R


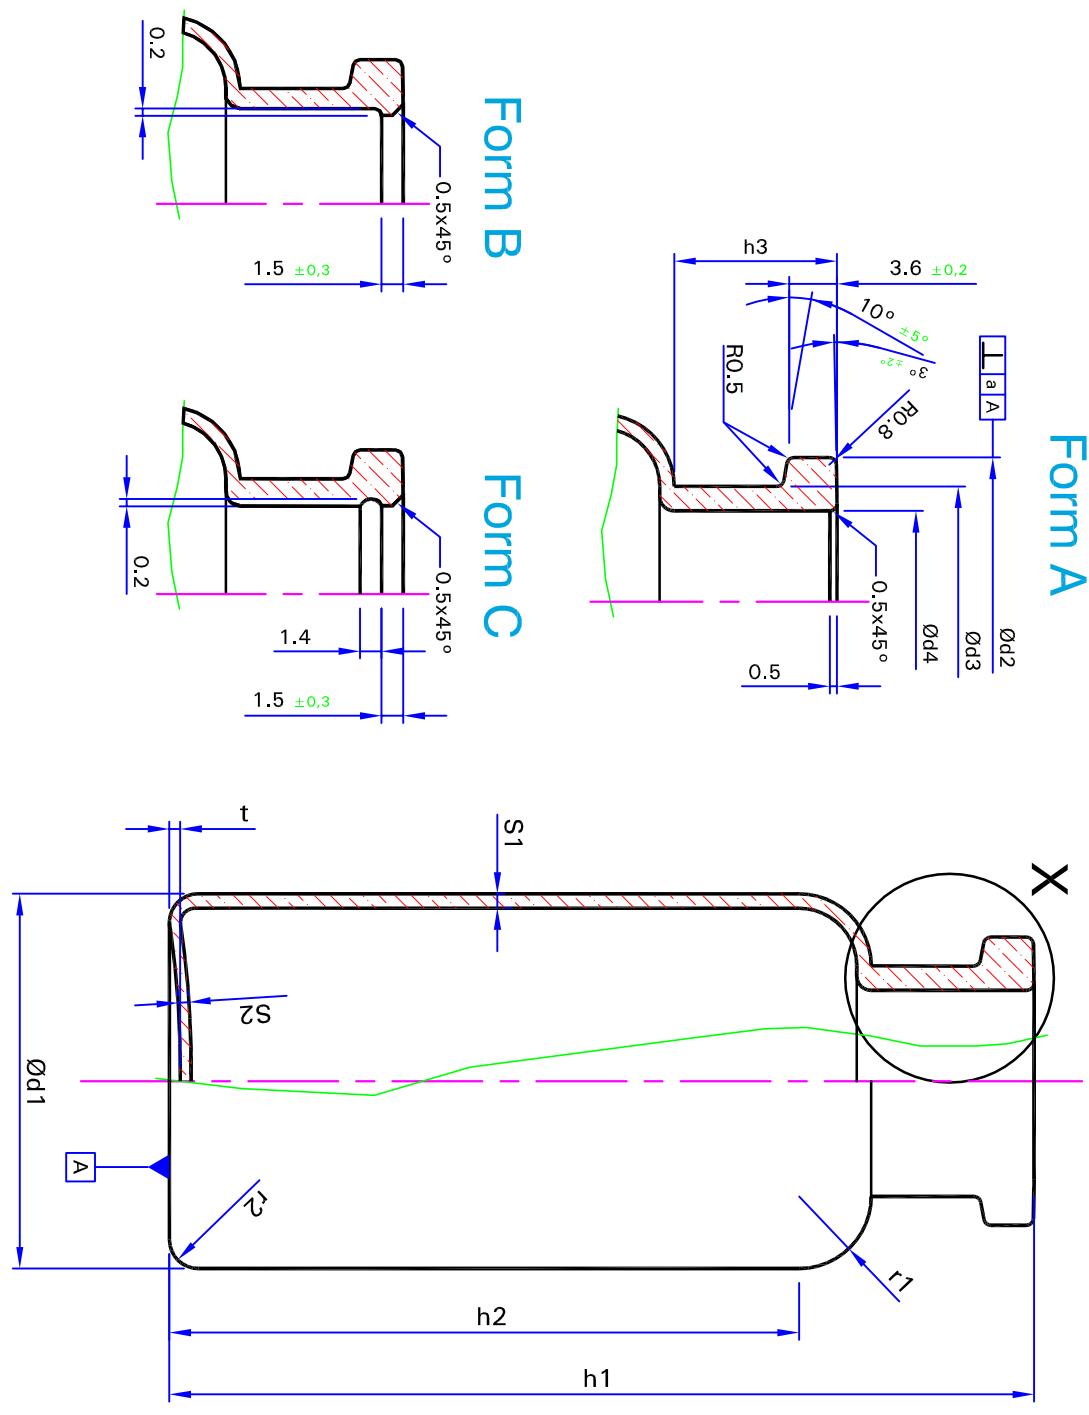


Table1

Nominal size	30R
Overflow capacity ml	37.5 ± 1.5
a	1.5
d1	30 ± 0.25
d2	$20^{+0.2}_{-0.3}$
d3	max. 17.5
d4	12.6 ± 0.2
h1	75 ± 0.7
h2	min. 55
h3	10 ± 0.75
r1	5.5
r2	2.5
S1	1.2 ± 0.05
S2	min. 0.7
t	max. 1

Vial ISO 8362-1:2009

Size designation of injection vial :30R

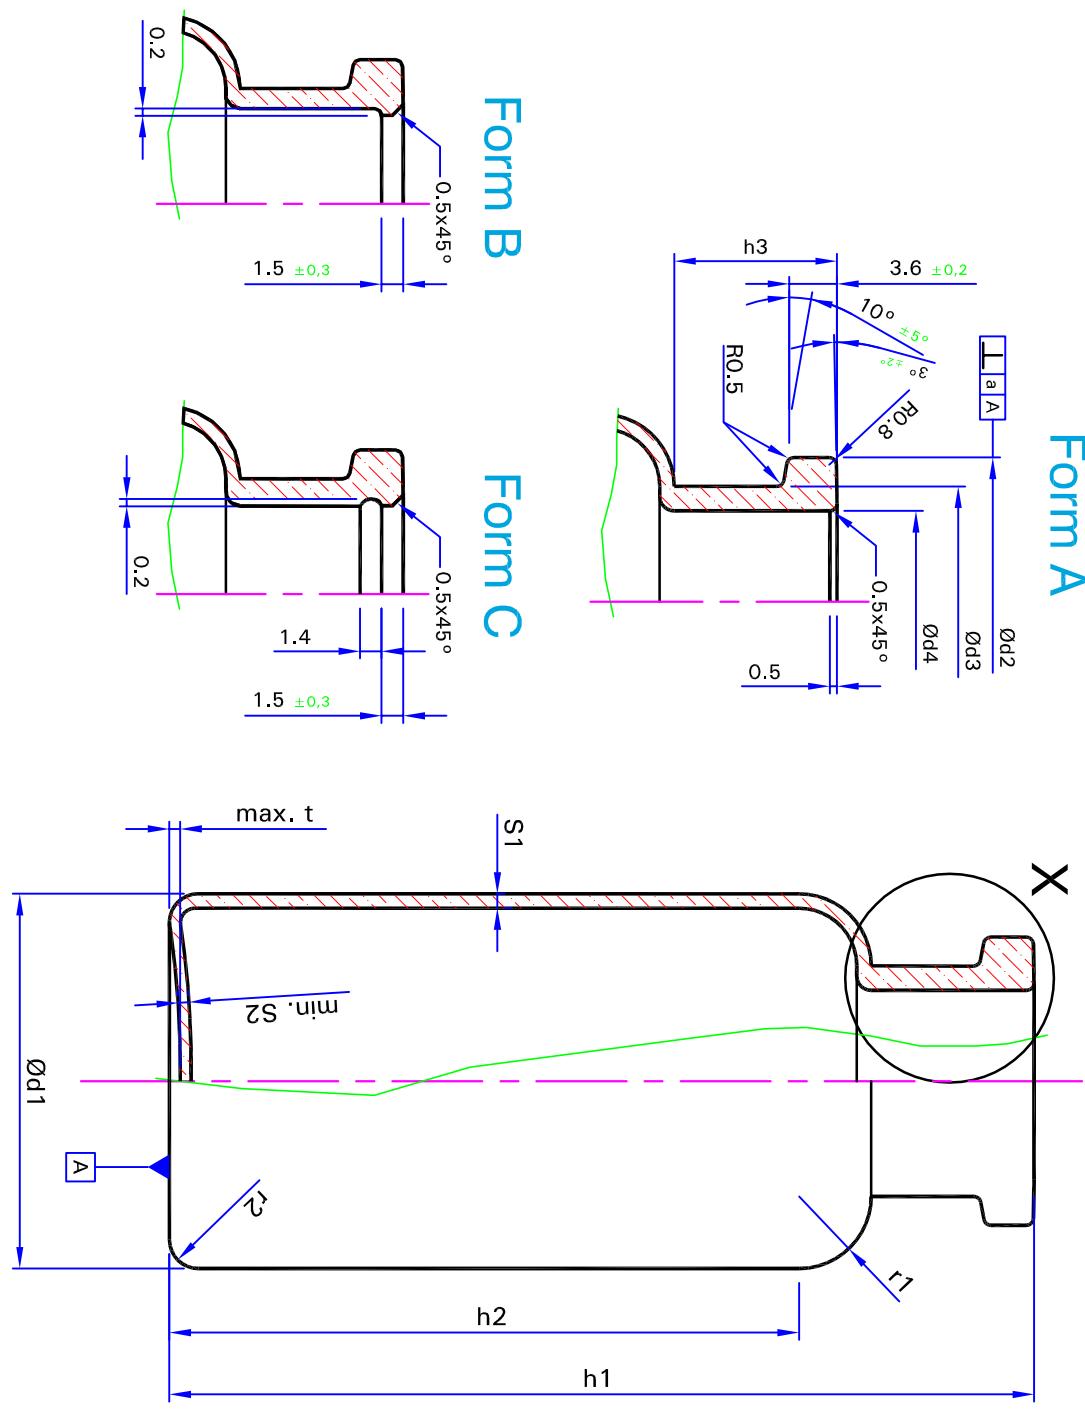

Injection vial